


## OLIS DSM 245

### CPL Solo plus Circular Dichroism

Measure your chiral molecules in both their ground and excited states using this one compact, all new spectrophotometry system. Think of it as an OLIS CD with CPL or as an OLIS CPL Solo with circular dichroism; both are correct. Single beam absorbance, fluorescence, polarization of fluorescence, circularly polarized luminescence, and circular dichroism. Two spectral ranges are available, UV optimized or red shifted.

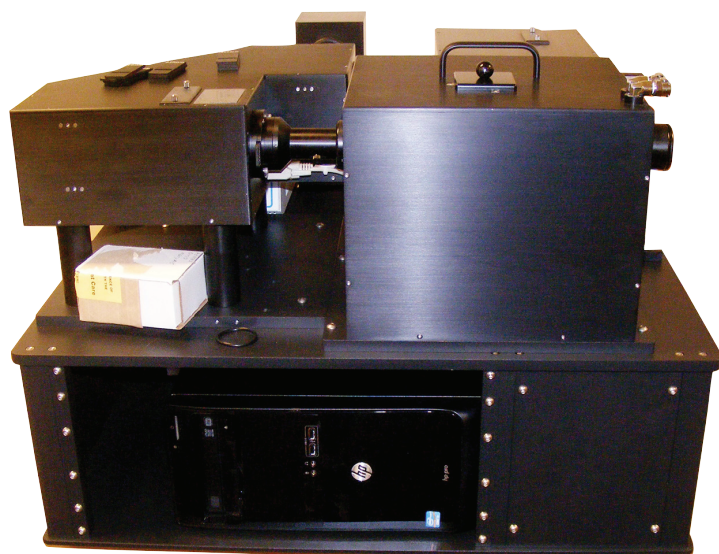

#### Standard Acquisition Mode:

**Absorbance**  
**Fluorescence**  
**Polarization of Fluorescence**  
**Circularly Polarized Luminescence**  
**Circular Dichroism**

#### Enhancements Supported:

CLARiTY  
 Phosphorescence Lifetime  
 Peltier Thermal Control  
 Thin Film Holder  
 Titrator

### OLIS DSM 245 SPECIFICATIONS

Light Source	150 watt xenon arc lamp for CD and CPL emission; UV optimized version uses UV coated lamp which requires N2 purging; optional LED for CPL excitation at chosen wavelength(s)
Monochromator 1	Subtractive double grating monochromator with two concave gratings for either 170-700 nm (UV) or 200-800 nm (red shifted) performance; very high stray light rejection and photometric accuracy. Used for CD; optionally used during CPL.
Monochromator 2	Single grating monochromator with single concave grating , used for 250-850 nm scanning during fluorescence and CPL.
Wavelength Range	170-700 nm or 200-800 nm for absorbance & CD; 250-870 nm for fluorescence & CPL
Spectral Bandwidth	0.5, 2.4, 5.0, 13 and 25 nm.
Wavelength Accuracy	± 0.2 nm
Monochromator Motor Step	0.125 nm/step
Integration Time	10 ms to 100 s
Wavelength Scanning Speed	2000 nm/min
Wavelength Slewing Speed	60 nm/sec
Acquisition Method	Digital Subtractive Method (DSM) for entirely digital data acquisition. Raw abs(L) and abs(R) are used for CD; raw fluor(L) and fluo(R) for CPL
G-Factor Acquisition	Not Required, because of DSM
Lock-in Amplifier	Not Required, because of DSM